

Radiation Dose and Image Quality Evaluation in Paediatric Radiography

A.P. Ladia, S.G. Skiadopoulos, C.P. Kalogeropoulou, P.E. Zampakis,
G.G. Dimitriou, G.S. Panayiotakis

Abstract—Chest and abdomen radiographs are the most common examinations in paediatric radiology. It is important to ensure that patient radiation dose is kept to low level without image quality degradation. In this work, the effective dose, risk and image quality were assessed in chest and abdomen radiography. Eighty children (40 boys, 40 girls) participated in the study and they were categorized in four age groups, according to their anatomical characteristics. The dose and risk were estimated utilizing the PCXMC 2.0 code. The image quality was assessed by two radiologists based on image features provided by the CEC guidelines. The mean effective dose value was 13 μ Sv and 34.6 μ Sv for chest and abdomen, respectively. The risk was slightly higher in the case of 1 y age group. Image quality values were similar for all age groups, with a slight increase in chest radiographs compared to abdomen radiographs. Improved image quality values were obtained for the processed images, for both chest and abdomen radiographs.

Index Terms— Abdomen Radiography, Chest Radiography, Radiation Dose, Image Quality

I. INTRODUCTION

Chest and abdomen radiographs are the most common examinations in paediatric radiology. The main advantages of chest and abdomen radiographs are the low cost and the high speed of acquisition and diagnosis. However, it is important to ensure that patient radiation dose is kept to low level, due to the increased children radiosensitivity and longer life expectancy [1] without degradation of the image quality (IQ).

Many studies have been reported dealing with patient dose, image quality or both, in paediatric radiography [2-6]. These studies refer either to film based systems, or computed radiography (CR) systems and highlight the fact that the effective dose (ED) and consequently the associated risk depend on the patient size [7].

A. P. Ladia, Department of Medical Physics, School of Medicine, University of Patras, Patras, 26504, Greece,

S. G. Skiadopoulos, Department of Medical Physics, School of Medicine, University of Patras, Patras, 26504, Greece,

C. P. Kalogeropoulou, Department of Radiology, School of Medicine, University of Patras, Patras, 26504, Greece,

P. E. Zampakis, Department of Radiology, School of Medicine, University of Patras, Patras, 26504, Greece,

G. G. Dimitriou, Department of Paediatric, School of Medicine, University of Patras, Patras, 26504, Greece,

G. S. Panayiotakis Department of Medical Physics, School of Medicine, University of Patras, Patras, 26504, Greece

In this study, the ED, risk and IQ for four age groups of children undertaken chest or abdomen radiographic examination, using a CR system, were evaluated, utilizing a Monte Carlo based code, the PCXMC 2.0.

II. PATIENTS AND METHODS

A. Patient Data

Eighty children (40 boys, 40 girls) who underwent chest or abdomen examinations participated in this study. The chest radiographs were posterior- anterior and the abdomen radiographs anterior- posterior projection. All examinations were performed using the GE Model MS 18S radiology unit with tube filtration 3.5 mm Al at 80 kVp, installed in the Karamandaneio Children Hospital of Patras. The children were categorized into four age groups (1, 5, 10, 15 y), according to their anatomical (weight and height) characteristics (see Table 1). Patient data (sex, age, weight, height, body mass index (BMI)) and exposure parameters (tube voltage, tube load, Focus Skin Distance (FSD)) were collected for both examinations (see Table 2 and 3).

B. Entrance Surface Dose

The most widespread indicator used in dose calculation is the Entrance Surface Dose (ESD). The x-ray tube output and the exposure parameters (tube voltage, tube load) were utilized to calculate the ESD values, using the equation [8]:

$$ESD = T.O \cdot \left(\frac{100}{FSD}\right)^2 \cdot tube\ load \cdot BSF \quad (1)$$

where T.O. is the output of the x- ray tube (in mGy/mAs) at 80 kVp at a distance of 1 m normalized, tube load is the product of the tube current (in mA) and exposure time (in seconds), FSD is the focus skin distance (in cm) and BSF is the back scatter factor. The value of BSF used was 1.3 [9]. The values resulted from equation 1 were compared with the corresponding ESD values, as estimated by the PCXMC 2.0 code, for each patient.

Radiation Dose and Image Quality evaluation in paediatric radiography

Table 1. Classification of children according to age, sex and examination.

age [y]	1		5		10		15		total
	girls	boys	girls	boys	girls	boys	girls	boys	
chest	5	5	4	6	4	6	5	5	40
abdomen	5	5	5	5	6	4	5	5	40

Table 2. Patients data and exposure parameters for chest radiographs.

age	weight		height		BMI	FSD	tube voltage		tube load	
[y]	[kg]		[cm]		[kg/m ²]	[cm]	[kVp]		[mAs]	
	range	mean	range	mean	mean	mean	range	mean	range	mean
1	8.0-10.5	9.40	72-85	78.7	15.19	124	79-82	79.9	1.62-2.3	1.94
5	17.0-19.0	17.70	104-110	106.6	15.60	151	79-82	80.0	3.22-4.3	3.72
10	27.0-33.0	31.50	131-143	131.0	16.12	151	79-83	80.6	5.01-6.0	5.46
15	49.0-59.0	49.00	158-174	158.0	19.26	160	80-90	83.8	6.09-6.9	6.45

Table 3. Patients data and exposure parameters for abdomen radiographs.

age	weight		height		BMI	FSD	tube voltage		tube load	
[y]	[kg]		[cm]		[kg/m ²]	[cm]	[kVp]		[mAs]	
	range	mean	range	mean	mean	mean	range	mean	range	mean
1	8.3-10.5	9.43	71-80	77.0	15.89	109	72-82	78.20	3.22-4.3	3.70
5	18.0-20.0	18.80	104-110	106.9	16.45	150	78-83	80.20	4.74-5.4	5.06
10	28.0-35.0	31.80	131-144	138.3	16.60	151	78-82	79.90	5.66-6.6	6.15
15	50.0-60.0	54.90	161-175	167.9	19.45	158	82-90	84.90	6.63-7.7	7.17

C. Dose and Risk Assessment

One common method for evaluating radiation dose is based on calculations using Monte Carlo techniques. The Monte Carlo based software PCXMC 2.0, developed at the Medical Radiation Laboratory of the Finnish Radiation and Nuclear Safety Authority, is a code for calculating patient doses in diagnostic radiology [10]. This code was used to calculate the dose of each organ separately, as well as the ED according to the equation [10-11]:

$$E = \sum_T W_T \left[\frac{H_T^M + H_T^F}{2} \right] \quad (2)$$

where W_T is the tissue weighting factor and H_T^M , H_T^F the equivalent doses for tissue T of male and female.

The ED value was used to estimate the risk for each patient undertaken chest or abdomen examination. For the assessment of risk resulting from an exposure to ionizing radiation [Risk of Exposure Induced cancer Death (REID)], the BEIRVII mathematical model was used [12].

The calculations were carried out using the Intel® Core™ 2 Duo processor of 2.66 GHz CPU powered by Asus and 4 GB installed memory (RAM). The calculation time required for each patient was 45 to 60 min. Statistical analysis was performed to investigate the correlation between patient dose and exposure parameters. Specifically, student t-test with threshold of statistical significance of 0.05 was used.

D. Image Quality Evaluation

To assess image quality and consequently the amount of diagnostic information received, a visual grading analysis of the radiographs was performed in accordance with the CEC guidelines, which define the acceptability of radiographs [13]. The visibility of the image features was assessed using a five-grade scale (see Table 4), enabling quantitative evaluation of the image quality criteria. Two radiologists, experienced in reading radiographs, interpreted the images in a random order, independently and blinded to the technique

Table 4. Grading scale for image quality criteria.

Grade	Definition
1.	Criterion definitely not fulfilled
2.	Criterion probably not fulfilled
3.	Not sure whether criterion fulfilled or not (50-50)
4.	Criterion probably fulfilled
5.	Criterion definitely fulfilled

used. In total, 80 radiographs were evaluated. During reading the room illumination was dimmed and kept constant, while reading time and radiologist to monitor distance were not restricted. The image quality assessment criteria (see Tables 5 and 6) used were based on the CEC guidelines [14]. The maximum possible total image quality score for each image was 65 for chest radiographs and 25 for abdomen radiographs, if all criteria were applicable. The final total score for each image was acquired by summing the mean scores of the two observers for each image feature. The whole procedure was repeated for all images after processing of the images using the ImageJ tool [15].

Table 5. Image quality criteria for chest radiography.

Assessment of Image Quality for chest radiographs	
1.	Performed at peak of inspiration, except for foreign body aspiration
2.	Reproduction of the thorax without rotation
3.	Reproduction of the thorax without tilting
4.	Reproduction of the chest must extend from just above the apices of the lungs to T12/L1
5.	Reproduction of the vascular pattern in central 2/3 of the lungs
6.	Reproduction of the trachea
7.	Reproduction of the proximal bronchi
8.	Visually sharp of the diaphragm reproduction
9.	Visually sharp of costo-phrenic angles
10.	Reproduction of the spine
11.	Reproduction of par spinal structures and visualization
12.	Reproduction of the retro cardiac lung
13.	Reproduction of the mediastinum

Table 6. Image quality criteria for abdomen radiography.

Assessment of Image Quality for abdomen radiographs	
1.	Reproduction of the abdomen, from the diaphragm to the inchiial tuberosities including the lateral abdominal walls
2.	Reproduction of the properitoneal fat lines consistent with ages
3.	Visualization of the kidney outlines consistent with age and depending on bowel content
4.	Visualization of the psoas outlines consistent with age and depending on bowel content
5.	Visually sharp reproduction of the bones

E. Statistical Analysis

Reliability analysis [16] was utilized in order to assess the agreement between the IQ scores of the two radiologists (inter-observer agreement) in 80 chest and abdomen radiographs. Furthermore, to assess the agreement between the IQ scores of the same radiologist (intra-observer agreement), 30 chest and abdomen radiographs were analysed. Intraclass correlation coefficient [ICC] and its corresponding 95% confidence interval [CI] were calculated for initial and processed chest and abdomen radiographs. The degree of agreement was scaled as almost perfect (ICC = [0.81-1.00]), substantial (ICC = [0.61-0.81]), moderate (ICC = [0.41-0.61]), or weak (ICC = [0.21-0.41]) [16]. Statistical analysis was performed using the IBM SPSS Statistics software package (SPSS Release 22.0, SPSS Inc., and Chicago, IL, USA).

Inter-observer agreement of radiologists was substantial for initial radiographs (ICC=0.706, CI= [0.577-0.801]) and moderate for processed radiographs (ICC=0.573, CI= [0.406-0.703]). Intra-observer agreement of radiologists was perfect for both radiologists, for both initial radiographs (ICC=0.948, CI= [0.878-0.978]; ICC=0.940, CI= [0.863-0.975], respectively) and processed radiographs (ICC=0.935, CI= [0.849-0.972]) and (ICC=0.881, CI= [0.731-0.949], respectively).

III. RESULTS

Table 7 presents the mean ESD in chest examinations for all age groups, as calculated using the equation 1 and the PCXMC 2.0 code, together with corresponding values published in other studies [17-20], as well as with the Diagnostic Reference Levels (DRLs) reported by National Radiological Protection Board [21]. Table 8 presents the corresponding ESD values of our results and published values

Table 7. Comparison of mean ESD values with other studies and NRPB DRLs for chest examinations.

Age [y]	This study (eq.1)	ESD (μGy) for chest					NRPB DRLs
		This study (PCXMC2.0)	Morales et al	Kiljunen et al	Compagnone et al	Nahangi et al	
1	76	78	86- 87	40	-	81	80
5	89	86	90- 88	60	29	122	110
10	94	95	78- 78	110	-	170	70
15	107	109	-	180	-	213	110

Table 8. Comparison of mean ESD values with other studies and NRPB DRLs for abdomen examinations.

Age [y]	This study (eq.1)	ESD (μGy) for abdomen					NRPB DRLs
		This study (PCXMC 2.0)	Morales et al	Kiljunen et al	Compagnone et al	Nahangi et al	
1	195	201	-	220	-	587	340
5	290	312	-	280	413	1088	590
10	470	511	-	660	-	1475	860
15	955	960	-	630	-	2202	2010

for abdomen examinations. It worths to notice that the ESD values derived by equation 1 and PCXMC 2.0 code were practically the same. For chest radiographs, the ESD values in our study for 1 and 15 y were slightly lower than DRLs and value of other studies, except to the values reported by Kiljunen et al. The ESD values for the 5 y group in our study were higher than the values reported by Kiljunen et al. and Compagnone et al., but lower than the DRLs and the value of other studies. The ESD values for the 10 y group in our study were higher than the DRL values and the values reported by Morales et al., but comparative to the values reported by Kiljunen et al. and lower than the value reported by Nahangi et al. For abdomen radiographs, the ESD values, of our study were lower than the DRL values, as well as the values reported by other studies except the values reported by Kiljunen et al.

Table 9 presents the mean ED and REID values for all patient groups for chest and abdomen radiography. The mean value of ED for all paediatric patients studied was 13 μSv and 34.6 μSv for chest and abdomen, respectively. The mean value for ED was up to three times higher for abdomen compared to chest radiography. As expected, the minimum ED value was estimated in the case of 1 y age group, 11.9 μSv and 32 μSv for chest and abdomen radiography, respectively. For the same age group the highest REID value was estimated $0.721 \cdot 10^{-5}$ and $1.321 \cdot 10^{-5}$ for chest and abdomen, respectively. This occurred due to the higher radiosensitivity of tissue and the longer life expectancy of the certain group. In general, the REID values were almost double for abdomen compared to chest examination for all paediatric patient groups.

Table 10 presents the IQ score for chest and abdomen radiographs before and after image processing. The IQ score obtained was slightly higher for the chest radiographs (4.1-

4.5) compared to the abdomen radiographs (4.1- 4.2), while for the processed radiographs were 4.3- 4.6 for chest and 4.2- 4.3 for abdomen radiographs. That increase was statistically significant for both examinations.

Table 9. Mean ED values and REID values for chest and abdomen examinations.

age [y]	Effective dose (μSv)		REID • 10 ⁻⁵	
	chest	abdomen	chest	abdomen
1	11.9	32.0	0.721	1.321
5	12.9	34.0	0.695	1.172
10	13.5	35.7	0.638	1.107
15	13.8	36.5	0.601	1.092
total value	13.0	34.6	0.664	1.173

Table 10. Mean IQ values for all patient groups for chest and abdomen radiographs.

age [y]	IQ initial		IQ processed	
	chest	abdomen	chest	abdomen
1	4.5±0.3	4.1±0.2	4.6±0.2	4.3±0.1
5	4.2±0.3	4.1±0.1	4.4±0.2	4.2±0.1
10	4.1±0.3	4.1±0.2	4.3±0.2	4.3±0.1
15	4.2±0.3	4.2±0.2	4.4±0.3	4.3±0.1
total value	4.3±0.3	4.1±0.2	4.4±0.2	4.3±0.1

Table 11. Comparison of ED values (mean and range) with other studies, for chest radiography.

age [y]	effective dose (μSv) for chest									
	This study		Shatskiy et al		Kiljunen et al		Compagnone et al		Nahangi et al	
	mean	range	mean	range	mean	range	mean	range	mean	range
1	11.9	11-13	40	10-130	7	3- 11	-	-	8	-
5	12.9	12-13	30	10-140	11	2- 27	5	1- 8	12	-
10	13.5	13-14	30	10- 80	18	2-121	-	-	17	-
15	13.8	13-14	30	10- 80	30	6- 73	-	-	19	-

Table 12. Comparison of ED values (mean and range) with other studies, for abdomen radiography.

age [y]	effective dose (μSv) for abdomen									
	This study		Shatskiy et al		Kiljunen et al		Compagnone et al		Nahangi et al	
	mean	range	mean	range	mean	range	mean	range	mean	range
1	32.0	31-33	120	20-440	56	6-263	-	-	94	-
5	34.0	33-35	140	30-440	72	8-281	102	68-134	193	-
10	35.7	35-36	340	140-680	144	8-267	-	-	255	-
15	36.5	36-37	550	220-1800	170	100-283	-	-	334	-

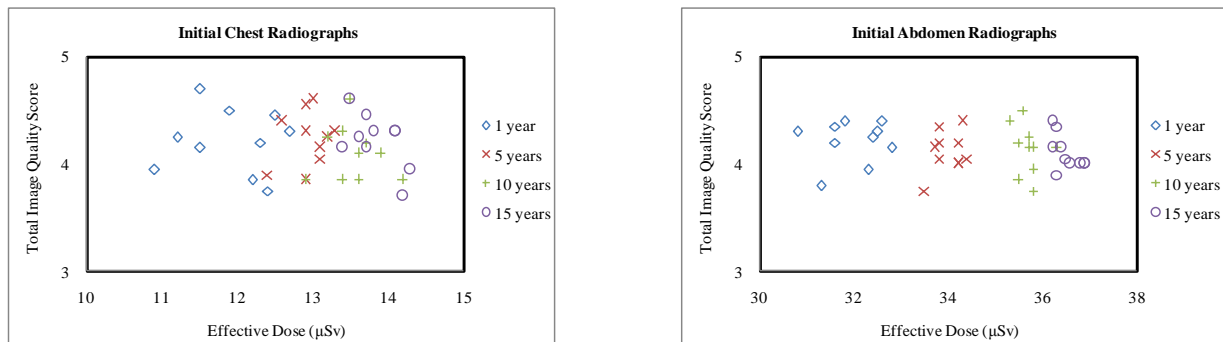


Figure 1. Total image quality score vs effective dose for the initial chest and abdomen radiographs.

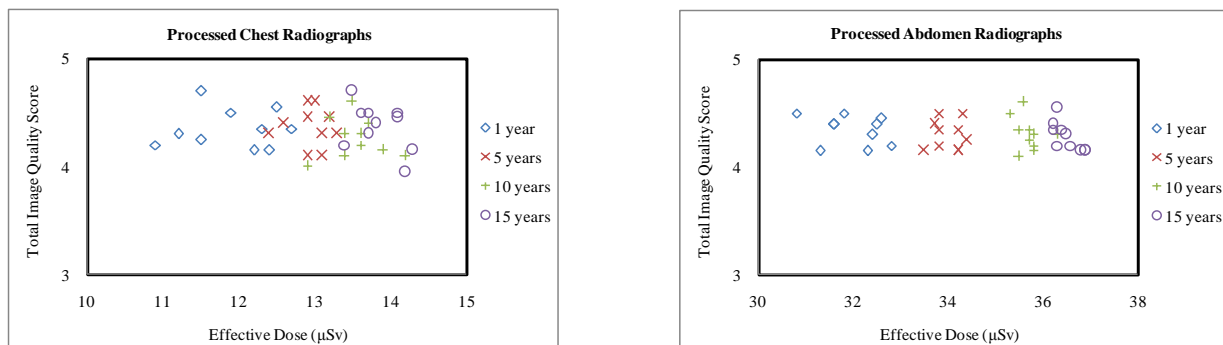


Figure 2. Total image quality score vs effective dose for the processed chest and abdomen radiographs.

IV. DISCUSSION

The ED values (mean and range) estimated in our study were compared with the corresponding values reported in similar representative studies [17-18, 20, 22], as shown in Table 11 for the case of chest radiographs and in Table 12 for

the case of abdomen radiographs. In general, the ED values for all age groups in our study were comparative or lower than those previously reported, for both chest and abdomen examinations. For chest radiography our results were

comparative to the values reported by Nahangi et al. and Kiljunen et al. for the group of age 1 and 5 y. For abdomen radiography our results were comparative to the values reported by Kiljunen et al. for the groups of age 1 and 5 y, whilst our results were lower or significant lower compared to the other values reported. Regarding image quality, the IQ score obtained was high in all cases. The IQ values were slightly higher for chest radiographs compared to abdomen radiographs. Even higher IQ values were obtained for the processed radiographs. Similar remarks are obtained from Figures 1 and 2, where the total IQ scores versus the mean ED values for initial and processed chest and abdomen radiographs are presented.

The main limitations of our study are the small number of patients for each age group and the fact that examinations were performed using only one radiographic unit.

V. CONCLUSIONS

The ED value was slightly increased with the age of the paediatric patients. The risk was slightly higher in the case of 1 y age group. The IQ values were similar for all age groups, with a slight increase in chest radiographs compared to abdomen radiographs. Improved IQ values were obtained for the processed images, for both chest and abdomen radiographs.

ACKNOWLEDGMENT

We would like to thank the staff of the Radiological Department of Karamandaneio Children Hospital of Patras for their assistance and cooperation during data collection.

REFERENCES

- [1] Committee on environmental health, "Risk of ionizing radiation exposure to children: A subject review", *Pediatrics*, vol. 101, 1998, pp. 717-719.
- [2] K.A. Gogos, E.N. Yakoumakis, I.A. Tsalafoutas, T.K. Makri, "Radiation dose considerations in common paediatric X-ray examinations", *Radiat. Prot. Dosim.*, vol. 33, 2003, pp. 236-40.
- [3] T.Makri, E. Yakoumakis, D. Papadopoulou, G. Gialousis, V. Theodoropoulos, P. Sandilos, E.Georgiou, "Radiation risk assessment in neonatal radiographic examinations of the chest and abdomen: a clinical and Monte Carlo Dosimetry study", *Phys. Med. Biol.* vol. 51, 2006, pp. 5023-5033.
- [4] E.D. Dougeni, H.B. Delis, A.A.Karatzas, C.P. Kalogeropoulou, S.G.Skiadopoulos, S.P. Mantagos, G.S.Panayiotakis. "Dose and image quality optimization in neonatal radiography", *Br. J. Radiol.*, vol. 80, 2007, pp. 807-815.
- [5] W. Veldkamp, L.J. Kroft, J. Geleijns, "Dose and perceived image quality in chest radiography", *Eur. J. Radiol.* vol. 72, 2009, pp. 209-217.
- [6] A. Ladia, G. Messaris, H. Delis, G. Panayiotakis, "Organ dose and risk assessment in paediatric radiography using the PCXMC 2.0", *IOP Conference Series* 637 012014, 2015.
- [7] H. Kim, M. Park, S.Park, H. Jeong, J. Kim, Y. Kim, "Estimation of absorbed organ doses and effective dose based on body mass index in digital radiography", *Radiat. Prot. Dosim.*, vol. 153, 2013, pp. 92-99.
- [8] K. Nfaoui, F. Bentayeb, O. Basraoui, A.C. Azevedo, "Evaluation of paediatric X-ray doses in Moroccan university hospitals", *Radiat. Prot. Dosim.*, vol. 142, 2010, pp. 238-243.
- [9] N. Petoussi-Hens, M. Zankl, G. Drexler, W. Panzer, D. Regulla, "Calculation of backscatter factors for diagnostic radiology using Monte Carlo methods", *Phys. Med. Biol.* vol. 43, 1998, pp. 2237-2250.
- [10] M. Tapiovaara, T. Siiskonen. "PCXMC A monte carlo program for calculating patient doses in medical x-ray examination" (2nd Ed.), STUK-A231 Helsinki, Finnish Centre for radiation and nuclear safety, 2008.
- [11] A. Servomaa, M. Tapiovaara, "Organ dose calculation in medical x ray examination by the program PCXMC", *Radiat. Prot. Dosim.*, vol. 80, 1998, pp. 213-219
- [12] BEIR VII "Health Risk from exposure to low levels of ionizing radiation", National Academy of Science, 2006.
- [13] B.M. Moores, "CEC quality criteria for diagnostic radiographic images- Basic concepts", *Radiat. Prot. Dosim.*, vol. 57, 1995, pp. 105-110.
- [14] Commission of European Communities "European Guidelines on Quality Criteria for Diagnostic Radiographic Images in Paediatrics", Luxembourg ECSC-EC-EAEC.
- [15] C.A. Schneider, W. Rasband, K. Eliceiri, "NIH Image to ImageJ: 25 years of image analysis", *Nat. Methods*, vol. 9, 2012, pp. 671-675
- [16] P. Shrout, J. Fleiss, "Intraclass correlations: uses in assessing rater reliability", *Psychol. Bull.*, vol. 86, 1979, pp. 420-428.
- [17] G. Compagnone, L. Pagan, C. Bergamini, "Effective dose calculation in conventional diagnostic x-ray examinations for adults and paediatric patients in a large Italian hospital", *Radiat. Prot. Dosim.*, vol. 114, 2005, pp.164- 167.
- [18] T. Kiljunen, A.Tietäväinen, T. Parviainen, A. Viitala, M. Kortensniemi, "Organ doses and effective doses in pediatric radiography: patient-dose survey in Finland", *Acta Radiologica*, vol. 50, 2009, pp. 114-124.
- [19] J. Morales, W. Jaramillo, J.A. Puerta, A. Arrieta, "A comparison of age-dependent entrance skin doses in pediatric chest exams with diagnostic reference levels for Antioquia region of Colombia", *Radioprotection*, vol. 47, 2012, pp. 575-582.
- [20] H. Nahangi, A. Chaparian, "Assessment of radiation risk to pediatric patients undergoing conventional X-ray examinations", *Radioprotection*, vol. 50, 2015, pp. 19-25.
- [21] NRPB- W40 "Doses to patient from x-ray examinations in the UK: 2000 review", National Radiological Protection Board, Chilton, UK, 2002.
- [22] I. Shatskiy, V. Golikov, "Paediatric doses in St Petersburg hospitals", *Radiat. Prot. Dosim.*, vol.165, 2015, pp. 199-204.